Instruction for use

IMM1056_IFU.Version8.2020-09-16





CloverFoot



Index

User manual – English3
Bruksanvisning - Svenska8
Bruksanvisning - Norsk 13
Brugervejledning - Dansk 18
Käyttöohjeet – Suomi 23
Gebrauchsanweisung - Deutsch 28
Gebruiksaanwijzing - Nederlands 33
Instruction d'utilisation – Francais37
Istruzioni per l'uso - Italiano 43
Instrucciones de uso - Español47

See www.etac.com



Thank you for choosing an Etac product.

To avoid accidents and injury when moving and handling the products, please read this manual carefully.

The person described as "the user" in this "Instruction for Use" is the person who is lying or sitting on the product. The carers are the people who manoeuvre the product.



This symbol appears alongside the text in the manual. It draws the reader's attention to points at which there may be a risk to the health and safety of the user or carer.

These products comply with the standards applicable for Class 1 products in the Medical Device Regulation (EU) 2017/745 on medical devices.


At Etac we strive to continually improve our products and therefore we reserve the right to make changes to products without prior warning. All measurements given on illustrations and similar material are for guidance only and Etac cannot be held liable for errors and defects. The information given in this manual, including recommendations, combinations and sizing, does not apply to special orders and modifications. If the customer makes adjustments, repairs or uses combinations not predetermined by Etac, the Etac CE certification and Etac warranty will not be valid. If in doubt, please contact Etac.

Warranty: Two-year warranty on material and manufacturing defects, provided that the product is used correctly.

Expected lifetime: The device has an expected service life of 1 to 2 years under normal use. The service life of the device varies depending on usage frequency, loads and how often and how it is washed.

For further information on the Etac Patient handling, see www.etac.com.

In case of an adverse event occurred in relation to the device, incidents should be reported to your local dealer and the national competent authority in a timely manner. The local dealer will forward information to manufacturer.

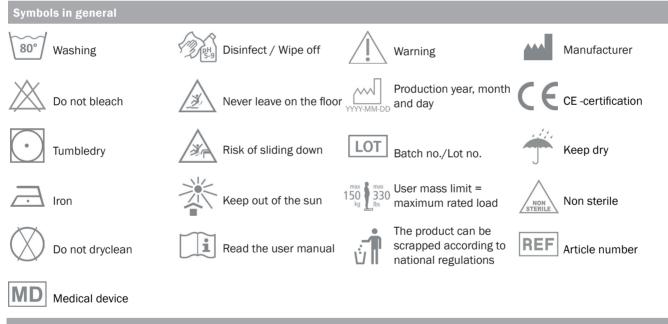

Intended use

CloverFoot is a footstool. It supports the user's feet when the bed, wheelchair or similar seat is not height-adjustable.

Intended environment

Acute care, Long-term care, Home care

 \square

Practical handling

Positioning

CloverFoot can be positioned where it is best for the individual user.

Use

The user will feel more secure when his/her feet are in contact with the floor, or, in this case, with the CloverFoot device.

Notice

Special features

Always check the product before use and after washing.

Never use a defective product. If the product shows signs of wear-and-tear, it must be scrapped.

Read these instructions carefully.

It is important that carers receive instruction in manual handling. Etac offers advice and training for carers. For further information, contact Etac.

Always use the correct manual handling techniques.

Encourage the user to assist where possible.

To ensure that the user feels safe and that every manual handling is smooth, always plan the manual handling in advance.

Material and cleaning

Material: Plastazote LD-45

The product should be checked regularly, preferably each time it is used, and especially after washing.

Check that there is no damage to the product.



Never try to repair a product yourself. Never use a defective product.

Never leave the product on the floor after use.

Always conduct a risk assessment, and ensure that the assistive product can be used for the individual user and, in combination with other devices, that it is safe for the user and carers.

If in any doubt - please contact Etac.

Washing instructions:

This product can be wiped off with soapy water or cleaned with a solvent-free cleaning agent with a pH level between 5-9, or a 70% disinfection solution.





Products and accessories

Article no.	Product Description	Size (mm)
IM2001	CloverFoot	W380xL320

Service information

Inspection

First inspection:

- Is the packaging intact?
- · Read the label on the packaging and check the article no. and product description
- Check that Short Instruction is enclosed updated User Manual/Instruction for use can be downloaded from www.etac.com or contact your Etac
 Customer Service or the local dealer.
- Check the label on the product does it include article no., product description, lot/batch no., cleaning instructions and supplier name?

Periodic Inspection:

- Make sure that your Manual transfer system always is in a perfect condition.
- After wash always check materials, stitching, handles, buckles.
- If the product shows signs of wear and tear, it must be removed from service immediately.

Visual inspection/Check the product: Ensure that the materials, seams, stitching, handles, buckles are intact/faultless.



Stability test:

Try to bend the product verify that it feels firm, stable and solid.



Mechanical load or stress/Test handles: Draw hard in the handles in opposite directions

and control the material, seams and stitching. Test buckles: Lock the buckle and draw in opposite directions, control the buckle and the stitching.



Test low/high friction:

Place the product on a firm surface or a bed, place your hands on the material and test the friction by pushing your hands down into the product.

Low friction – slides effortlessly High friction – no sliding/moving

Check:

Manual transfer aids with handles, straps and buckles:



Manual transfer aids with for sitting and lying transfer and with high or low friction:

KG KG

M

Production year, month and day



The product can be scrapped in accordance with national regulations

Ĺ

ш